

# System Requirements

---

- 1GHz or higher CPU
- 1GB or more RAM
- Hard disk with 2GB or more spare space
- USB 2.0/3.0

## The software supports the following operating systems:

- Microsoft Windows Vista
- Microsoft Windows 7
- Microsoft Windows 8
- Microsoft Windows 10

If the operating system is lower than the above version, please update the system first.

## Installation


---

1. Insert the installation CD into the CD-ROM of a computer.
2. The installation interface pops up. (If no installation interface appears, double-click Setup.exe in the CD-ROM directory to start it manually.)

## Using the Software


---

### 1. Interface

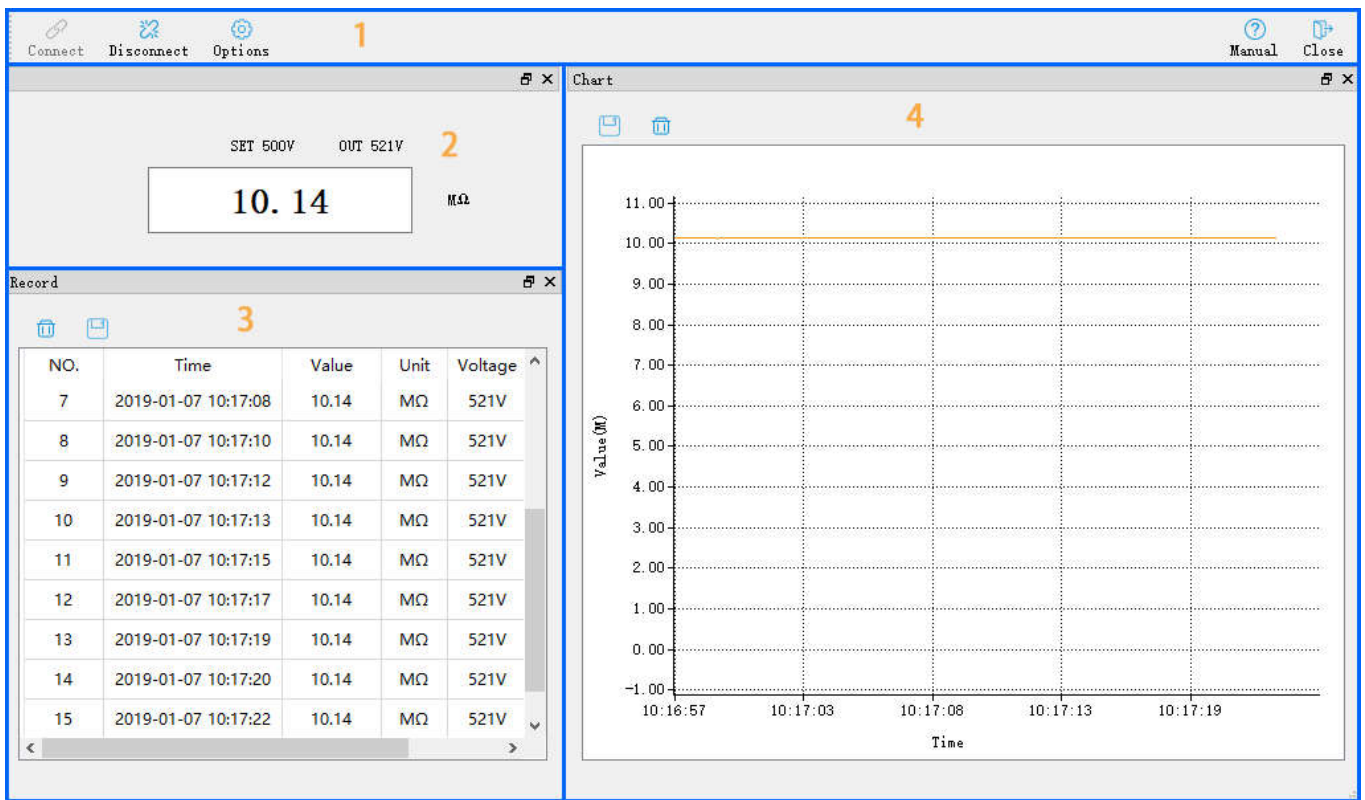

Area	Description
1	Toolbar
2	Real-time measurement
3	Data record
3	Data chart



## 2. Connecting device

- Click  Connect
- If the connection is successful, the measurement data will be displayed in Area 2, Area 3, Area 4.


## 3. Disconnect

- Click  Disconnect
- Each area will stop displaying measurement data


## 4. Export

- Click  in area 3 to export the data record to an Excel file
- Click  in area 4 to export the data record to an Jpeg file

## 5. Clear data


- Click  to clear the recorded data.

## 6. Close the software

- Click  to close the software

## 7. Setup software

- Click 

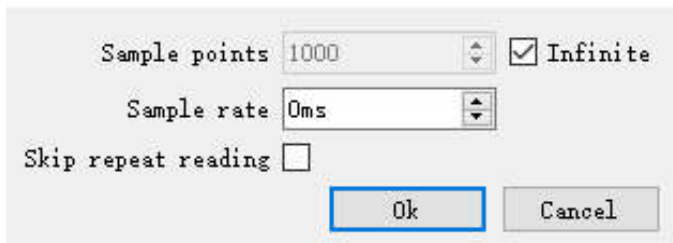

The image shows a dialog box titled "Options" with a gear icon. It contains three settings: "Sample points" set to 1000 with a checked "Infinite" checkbox, "Sample rate" set to 0ms, and "Skip repeat reading" which is unchecked. At the bottom are "Ok" and "Cancel" buttons.

Sample points	1000	<input checked="" type="checkbox"/> Infinite
Sample rate	0ms	
Skip repeat reading	<input type="checkbox"/>	

Ok Cancel

- "Sample Points": Set the number of sampling points. If "Infinite" is checked, the number is unlimited
- "Sample rate": Set the sampling rate. If the set rate is greater than the actual rate, the actual rate will prevail; if set to 0, the actual rate will be sampled
- "Skip repeat reading": If checked, the same sample value as the previous one is not recorded